

Transcend LX UHPLC Systems

Boost LC-MS throughput to a new level

The unique multichannel LC capability of the Thermo Scientific™ Transcend™ LX UHPLC systems increases throughput by up to four times, maximizing mass spectrometer productivity and return on investment. This multichannel LC capability also allows different methods to be run on separate channels simultaneously, reducing cross-contamination and downtime between method-switching. Transcend LX UHPLC Systems can be used with any Thermo Scientific™ mass spectrometer and also with other select mass spectrometers.


Benefits of multichannel LC technology

- Increases throughput and flexibility
- Decreases cost per sample
- Incorporates the leading precision of Thermo Scientific™ Vanquish™ Flex UHPLC pumps

Multichannel LC maximizes the utilization of your mass spectrometer and enhances your lab's return on investment


Use a two- or four-channel LC system in combination with a single mass spectrometer to increase LC-MS throughput, and enable a faster return on investment.

- Reduces mass spectrometer idle time
- Increases sample throughput without changing validated methods

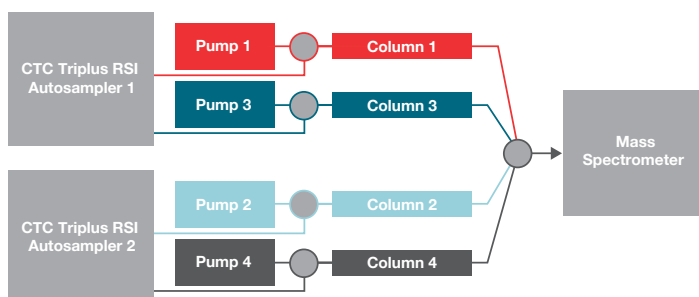

The Transcend LX systems feature either 2 or 4 (shown) completely independent LC channels.

The Thermo Scientific multichannel LC technology provides the throughput of up to four separate, parallel LC systems connected to a single mass spectrometer. With Thermo Scientific™ Aria™ MX software, each channel operates independently, so you can run a single method or multiple methods simultaneously. This critical feature improves MS efficiency, unlike traditional single-channel LC systems whose detectors are typically idle more than 75 percent of the time. Transcend UHPLC systems ensure efficient utilization of your mass spectrometer with dramatically reduced idle time. Save money effortlessly and boost sample throughput, without compromising data quality or sensitivity.

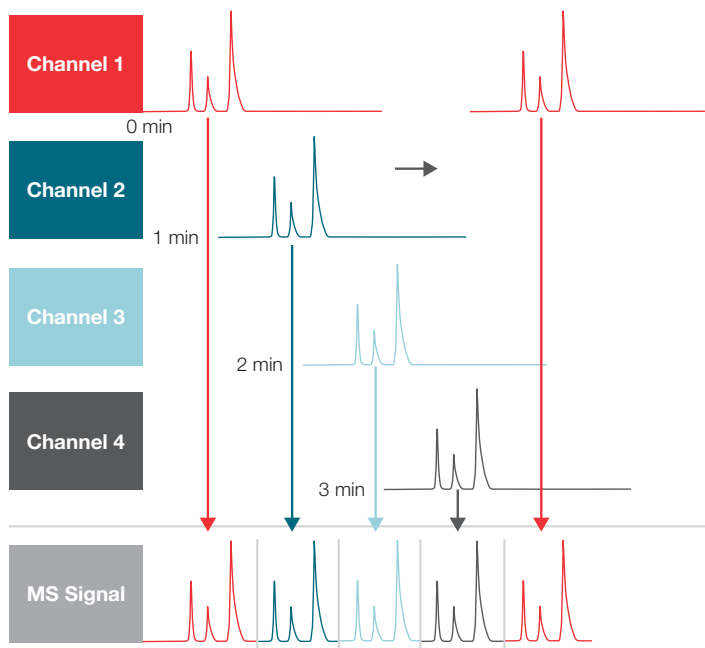

Injections are interleaved to maximize throughput and mass spectrometer utilization.



The Thermo Scientific™ Transcend™ LX-2 UHPLC System doubles throughput compared to a single LC system



The Thermo Scientific™ Transcend™ LX-4 UHPLC System—maximum throughput enabling four times the throughput of a single LC system.

Specifications

Transcend LX-2 UHPLC System (PN 60500-60207) and Transcend LX-4 UHPLC System (PN 60500-60208)	
Software	Aria MX software 2.6 or later Thermo Scientific™ Xcalibur™ 4.2 software or later Thermo Scientific™ Foundation™ platform 3.1 SP6 or later (Optional) Thermo Scientific™ TraceFinder™ 4.1 SP4 software or later
Solvent and additives	LCMS-grade solvents
Supported reservoir containers	0.25 L to 5 L with maximum height <350 mm
Pump (HPG)	2 Vanquish Binary Pump F (LX-2), 4 Vanquish Binary Pump F (LX-4)
Gradient Formation	High-pressure gradient proportioning
Flow range (Settable) [mL/min]	0.001–8, in 1 µL/min increments
Maximum pressure [bar]	1034 (103 MPa, 15,000 psi), linear decrease down to 800 (80 MPa, 11,600 psi) at flow rate >5 mL/min
Flow precision [% or µL min ⁻¹ or min]	<0.05% RSD or <0.01 min SD, whichever is greater
Flow accuracy [% or µL min ⁻¹]	±0.1%
Mixer volume [µL]	100 µL (includes 25 µL proprietary capillary mixer and 75 µL static mixer)
Dwell volume	100 µL
Pulsation [% or bar]	<1.0% or <2 bar, whichever is greater
pH range	2–12 (buffer or chloride concentration up to 1 mol/L)
Autosampler	Thermo Scientific™ TriPlus™ RSH Autosampler (LX-2: Single Head, LX-4: Dual Head) 80 cm Rail
Maximum pressure [bar]	1034 (103 MPa, 15,000 psi)
Carryover [%]	<0.003% with Chlorhexidine (600 µg/mL)
Sample capacity	2304 (well plate, 384 × 6 plates), 576 (well plate, 96 × 6 plates), 576 (6, 7 and 8 mm OD vial (≤1.2 mL), 96 × 6 racks), 324 (12 mm OD vials (≤2 mL), 54 × 6 racks)
Injection linearity [R ²]	>0.9999 (100 µL LCMS-P Tool)
Injection volume range [µL]	0.1–100
Maximum injection volume [µL]	100 (10 mL optional)
Temperature range [°C]	4–40
pH range	2–12
Injection precision 1	<0.1 % area RSD full loop injection (caffeine in water)
Injection precision 2	<0.5 % area RSD partial loop injection (caffeine in water)
Injection principle	Heart-Cut Loop Injection
Sample Extension	Optional CoolStack (3 drawer or 6 drawer 12MT)
Samples	4608 (well plate, 384 × 12 plates), 1152 (well plate, 96 × 12 plates), 1152 (6, 7 and 8 mm OD vial (≤1.2 mL), 96 × 12 racks), 648 (12 mm OD vials (≤2 mL), 54 × 12 racks) 12MT 6912 (well plate, 384 × 18 plates), 1728 (well plate, 96 × 18 plates)
Plate capacity	6 deep well plates or 12 well plates
Temperature range [°C]	4–40

Find out more at

thermofisher.com/TranscendMultichannelSystems