

8

7

6

5


4

3


2

1


REVISIONS			
REV.	DESCRIPTION	DATE	CHANGED BY
A	INITIAL RELEASE	12/22/2011	BARENDT
B	UPDATED REAR PANEL WITH MOUNTING BRACKET & HOLES; UPDATED DRAWING PER STANDARDS	03/16/2020	TFI

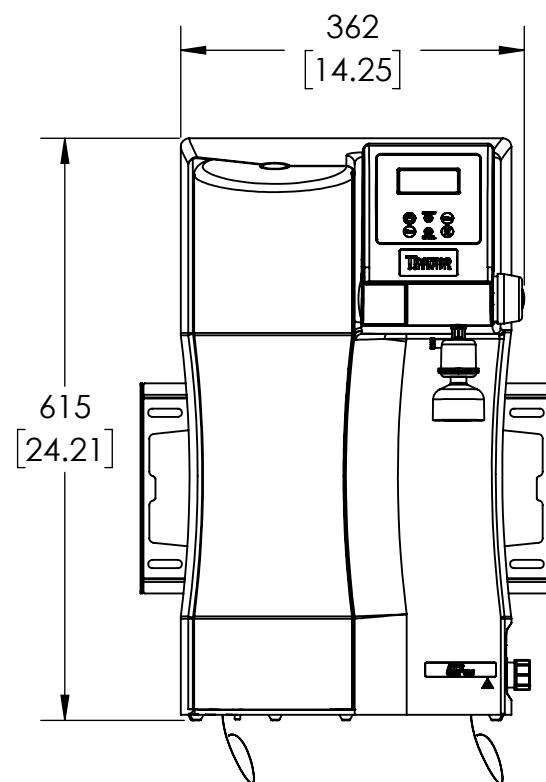

FRONT VIEW

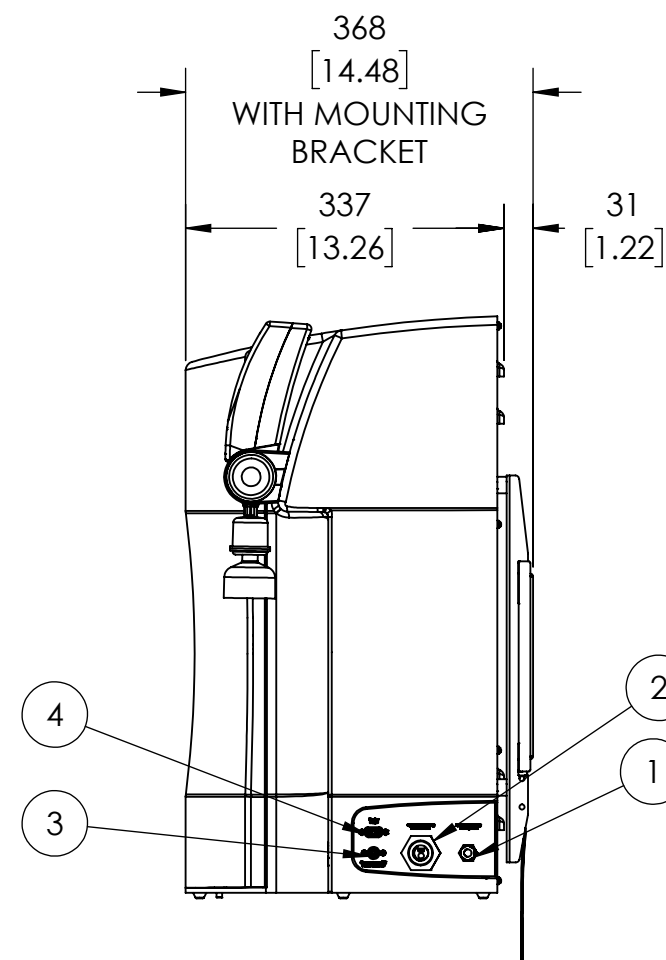

RIGHT SIDE VIEW

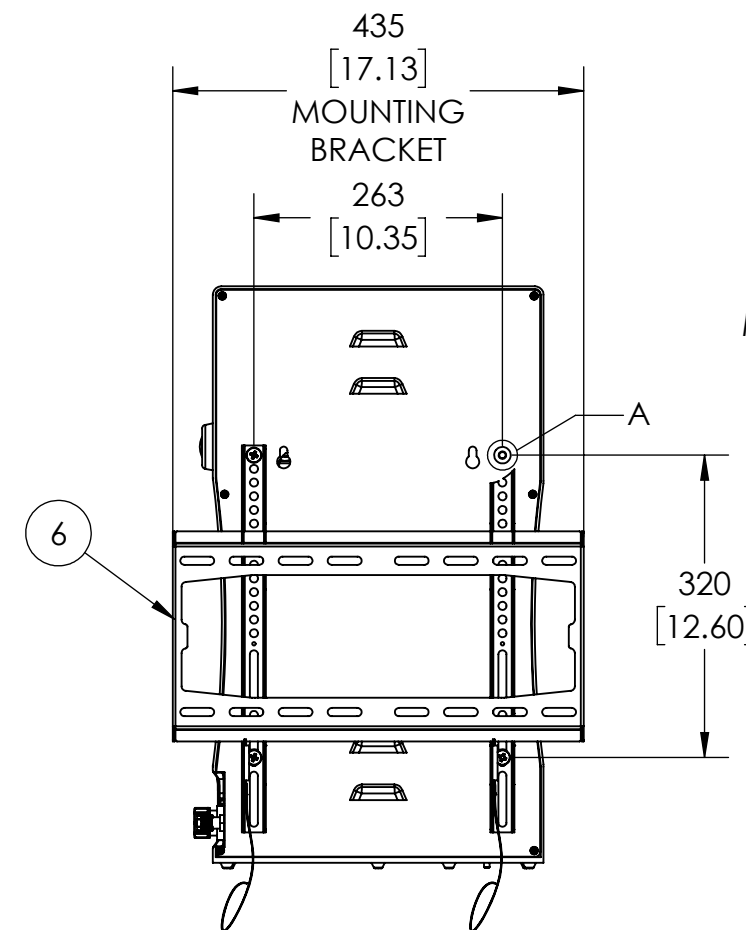

REAR VIEW

REAR PANEL MOUNTING- GENPURE

M8 PEM NUT

DETAIL A
4 PLACES

LEGEND:

1. RINSING WATER CONNECTION HOSE \varnothing 8MM
2. FEED WATER CONNECTION R3/4"
3. POWER SUPPLY CONNECTION 24V DC
4. PRINTER CONNECTION
5. HOLES FOR WALL MOUNTING BRACKET, 50157885
6. OPTIONAL WALL MOUNTING BRACKET, 50157885

NOTES:

1. DUAL DIMENSIONS ARE METRIC OVER INCH.
2. ENSURE THAT THERE IS ADEQUATE SPACE ALL AROUND THE UNIT APPROX. 30CM (11.8 INCH) FOR CONSUMABLE REPLACEMENT.

ELECTRICAL REQUIRMENTS	100-240 V, 50/60Hz, 2-1A, UPTO 1.5M (5 FEET) FROM UNIT
WATER CONNECTIONS	3/4" NPT WITH MANUAL SHUT OFF VALVE RECOMMENDED
MIN/MAX INLET PRESSURE	2-87 PSI(0.1-6 BAR)
RECOMMENDED FEED TEMPERATURE	2-40 °C
RECOMMENDED FEED WATER TYPE	PURE WATER (TYPE 2 WATER)
DRAIN	AN ATMOSPHERIC DRAIN MUST BE AVAILABLE WITHIN 1.5M(5 FEET) OF THE UNIT
UNIT DRY WEIGHT	53 lb (24 KG)

CONFIDENTIAL INFORMATION		DO NOT SCALE DRAWING	DATE	ThermoFisher 22 Alpha Road Chelmsford, MA 01824 SCIENTIFIC
THIS DRAWING AND ALL INFORMATION AND FEATURES CONTAINED HEREIN ARE AND SHALL REMAIN THE EXCLUSIVE PROPERTY OF THERMO FISHER SCIENTIFIC. SHALL BE HELD CONFIDENTIAL, AND SHALL NOT BE REPRODUCED, COPIED, OR OTHERWISE DISPOSED OF, IN WHOLE OR IN PART, WITHOUT THE PRIOR WRITTEN PERMISSION OF THERMO FISHER SCIENTIFIC.		CREATED BY BARENDT	12/22/2011	
RoHS COMPLIANCE		CHECKED BY OPP	12/22/2011	TITLE DIMENSION DRAWING GENPURE
ALL PARTS, COMPONENTS, MATERIALS AND PROCESSES MUST BE CERTIFIABLY RoHS COMPLIANT ACCORDING TO CURRENT WORLD STANDARDS. ANY DEVIATION FROM THE RoHS STANDARD MUST BE SUBMITTED TO THERMO FISHER SCIENTIFIC ENGINEERING FOR APPROVAL PRIOR TO THE MANUFACTURING, PURCHASING AND ASSEMBLY OF ANY AND ALL PARTS, COMPONENTS, MATERIALS AND PROCESSES.		UNLESS OTHERWISE SPECIFIED, SURFACE ROUGHNESS SHALL BE: <input checked="" type="checkbox"/>		SIZE B
THIRD ANGLE PROJECTION		SCALE: 1:8		DWG. NO. MB083
		SHEET 1 OF 1		REV. B

8

7

6

5

4

3

2

1