


Reduce uncertainty and variation of measurements

Challenges

TEM image distortion occurs through lens aberrations and camera imperfections in electron optics.


A combination of distortion correction and magnification calibration specifications are needed to ensure repeatable, reliable measurements.

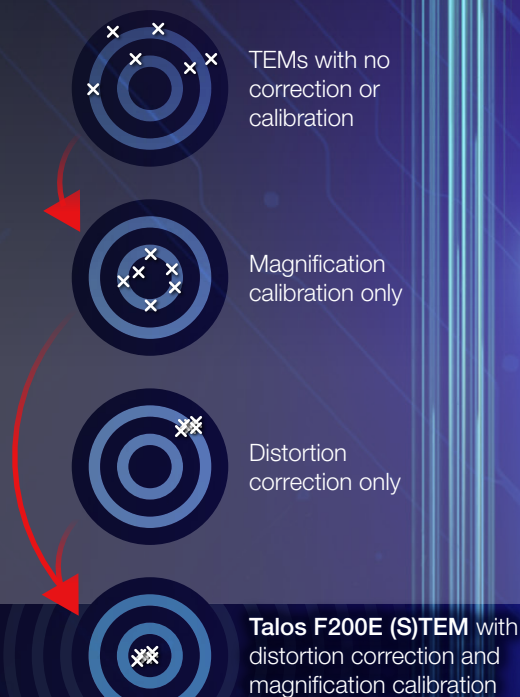

Talos F200E (S)TEM

Engineered to minimize causes of distortion.

The Thermo Scientific™ Talos™ F200E (S)TEM guarantees low tolerances for image distortion in TEM and STEM.

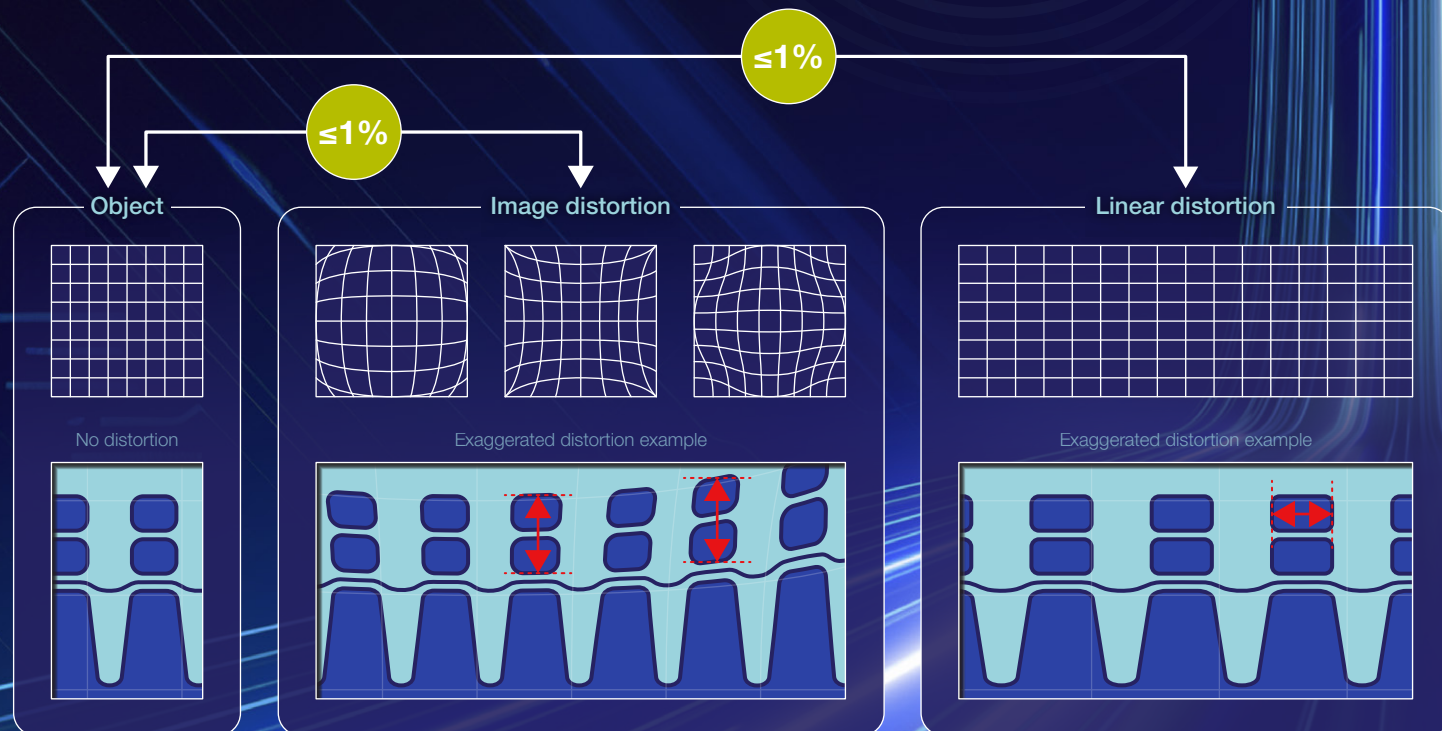

Learn more at thermofisher.com/talos

thermo scientific

For research use only. Not for use in diagnostic procedures. For current certifications, visit thermofisher.com/certifications

© 2025 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified.